AlcoMate Prestige (Model AL6000)
USER'S MANUAL

The AlcoMate Prestige is intended to measure alcohol in human breath. Readings obtained by this device are used in the diagnosis of alcohol intoxication. The accuracy of this device has been established at a Blood Alcohol Concentration of 0.008 and 0.032. Accuracy at a Blood Alcohol Concentration greater than 0.032 has not been evaluated. Accuracy testing was completed according to DOT regulations.

The AlcoMate Prestige (Model AL6000) analyzes a breath sample to detect alcohol in the lungs. This reading is then converted to blood alcohol concentration (BAC). The AlcoMate Prestige uses an advanced oxide semiconductor sensor to detect alcohol. **The Prestige is the first and only breathalyzer that features Pre-Calibrated Alcohol Sensor Modules to eliminate the need for recalibration. Just snap out, snap in and you're ready to go!**

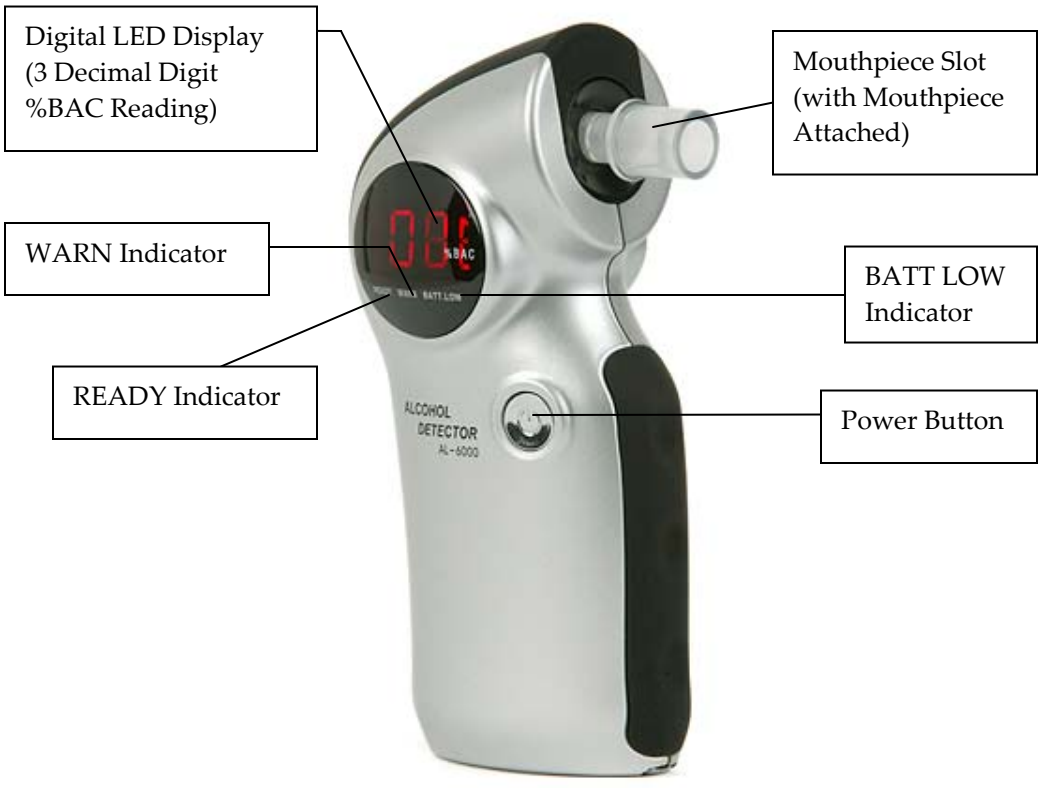

Device Operation

If you are using the Prestige for the first time, please install two 1.5V AA batteries (included) and attach a mouthpiece to the unit.

1. Instructions

a) Press and hold the Power Switch to turn the unit on. The cumulative test count will be displayed as you hold the Power Switch down.

b) Release the Power Switch. There will be a countdown from to as the unit warms up.

c) Secure your lips around the mouthpiece and blow sharply and steadily into the unit for about 4 seconds. You will hear two beeps when the device is done taking the breath sample. You will see the digit moving left to right in the display as the device analyzes the sample.

d) When analysis is complete, you will see the blood alcohol concentration (BAC) results displayed.

c) The results will be shown for about 15 seconds. The unit will then shut itself off.

d) If the device cannot take a successful sample, you will see in the display and the unit will shut itself off.

2. Understanding Your Results (BAC Reading)

Note: The AlcoMate Prestige uses a 3 Decimal Digit high-precision display. Rather than a reading such as "0.08%" the Prestige will display ".080%".

Your Reading	Your Range	Description	Device Behavior
.000% to .010%	Safe range.	Little/no alcohol intake.	(No special warnings.)
.011% to .049%	Moderate* range.	Increased alcohol intake.	(No special warnings.)
.050% and over	Warning* range.	Ability to drive may be impaired.	**Flashing WARN indicator and repeating beep.**

* *Drinking alcohol in ANY amount may impair the ability to drive. There is no "safe" level of alcohol intake before driving. Don't drink and drive.*

Note: The maximum reading the device can show is 0.400%. A true BAC of 0.400% or above may result in the onset of coma or even death by respiratory arrest. A reading of 0.400% may indicate an acutely dangerous condition, but may also indicate a sampling error (such as liquid alcohol blown into the device). Please carefully read the **Warnings** section of this manual before operating the device.

General Information about DUI/DWI

The legal limit for intoxication (DUI/DWI) has recently been lowered from 0.10% to **0.080%** BAC across most of the USA. According to the American Medical Association (AMA), a BAC of **0.050%** is enough to impair the ability to drive. *You should never operate a motor vehicle when you are impaired by the consumption of alcohol, drugs or lack of proper rest.*

Warnings

a. Wait at least 20 minutes after eating or drinking before testing. Alcohol remaining in the mouth, or even excess saliva, may interfere with testing. This includes alcohol-based mouthwash or similar products.
b. Avoid testing in high wind or enclosed spaces. Poor ventilation may also lengthen the time required for warm up between tests.
c. Do not blow smoke, saliva or other contaminants into the mouthpiece, as the sensor may become damaged.
d. Do NOT use the AlcoMate Prestige as a tool to drink and drive.
e. Keep out of extreme temperatures and out of the reach of children.
f. To maintain accuracy, we recommend replacing the alcohol sensor module inside the AlcoMate Prestige approximately every 300 tests, or if damaged by improper testing or handling.
g. **WARNING DISPLAY "Flo"**: If you see "Flo" in the display, the breath sample was not strong enough for measurement. Please try again and make sure the breath is strong and steady during sampling.
h. **WARNING DISPLAY "Cal"**: If you see "Cal" in the display, the unit requires recalibration or maintenance. Please use the contact information at the end of this document.
i. **WARNING DISPLAY "Bat"**: If you see "Bat" in the display, the battery power is low. Please replace the batteries.

Remove the battery cover at the bottom of the unit and replace the old batteries with two new 1.5V "AA" batteries. Make sure to properly align the batteries by looking at the +/- marks.

Specifications

Method of Measure	Breath sample to BAC
Range	0.000% to 0.400%
Accuracy	+/-0.010% up to 0.100% BAC
Sensor	Oxide semiconductor
Power	Two 1.5V AA alkaline batteries (included)
Testing Capacity	Approx. 200-300 with new batteries
DOT Approved	YES
Operating Temperature	10 – 40 degrees Celsius
Warm Up	Less than 1 minute
Display	3-Digit Decimal (.000)
Size (mm)	125 (height) X 58 (width) X 41 (thickness)
Weight	117 g
Sensor Modules	Sensor modules should be replaced approx. 200~300 tests, or if damaged by improper testing or handling

Warranty

The manufacturer warrants the product to be free from defects in workmanship or material (excluding calibration) under normal use for six (6) months from the date of purchase. The manufacturer's obligation under this warranty is limited to replacing, adjusting or repairing the unit if returned along with proof of purchase. This warranty is void if the unit has been tampered with or maliciously damaged.

Recalibration & Service

For recalibration and technical support, please contact us at:

American Screening Corporation
"Complete Drug Testing Solutions"
6658 Youree Dr Ste 180 PMB 404
Shreveport, LA 71105
Ph: 318-227-4994
Fax:318-227-4996
Toll Free: 1-866-526-2873
www.americanscreeningcorp.com